



## INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification <sup>7</sup> : <b>A61B 1/12, 1/00</b>	<b>A1</b>	(11) International Publication Number: <b>WO 00/40139</b> (43) International Publication Date: <b>13 July 2000 (13.07.00)</b>
---	-----------	--

(21) International Application Number: **PCT/US00/00109**

(22) International Filing Date: **4 January 2000 (04.01.00)**

(30) Priority Data:  
**09/227,244** **8 January 1999 (08.01.99)** **US**

(71) Applicant: **ORIGIN MEDSYSTEMS, INC. [US/US]; 135 Constitution Drive, Menlo Park, CA 94025 (US).**


(72) Inventors: **CHIN, Albert, K.; 2021 Newell Road, Palo Alto, CA 94303 (US). LUNSFORD, John, P.; 123 Leslie, San Carlos, CA 94070 (US). CHANG, Tenny; 151 Calderon #142, Mountain View, CA 94041 (US). BAXTER, Jeffrey, W.; 4731 Fordwell Drive, San Jose, CA 95118 (US).**

(74) Agents: **RAO, Dana, S. et al.; Fenwick & West LLP, Two Palo Alto Square, Palo Alto, CA 94306 (US).**

(81) Designated States: **AE, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, TJ, TM, TR, TT, UA, UG, UZ, VN, YU, ZA, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SL, SZ, TZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).**

**Published***With international search report.**Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.***(54) Title: CANNULA PROVIDED WITH IRRIGATION MEANS****(57) Abstract**

A retractor (112) and a surgical tool are positioned within a cannula (100), and a dissection cradle (116) of the retractor is positioned at the distal end of the cannula. The retractor includes a first portion (110) with an axis approximately parallel to the axis of the cannula and a second portion (114) with an axis skewed relative to the axis of the cannula. The dissection cradle may include two substantially parallel, spaced legs (141, 142) with the retractor shaped in a loop between and in a plane skewed relative to the axes of the legs, and with the loop directed away from the surgical tool. One of the legs supporting the retractor is hollow (1100) and includes a spray nozzle (1104) disposed in the distal end of the retractor to form an irrigation system. The spray nozzle on the retractor may be positioned to wash the endoscope lens, or upon selective extension of the retractor out of the cannula, the spray nozzle may be positioned to direct the spray of irrigation fluid at a remote surgical site.

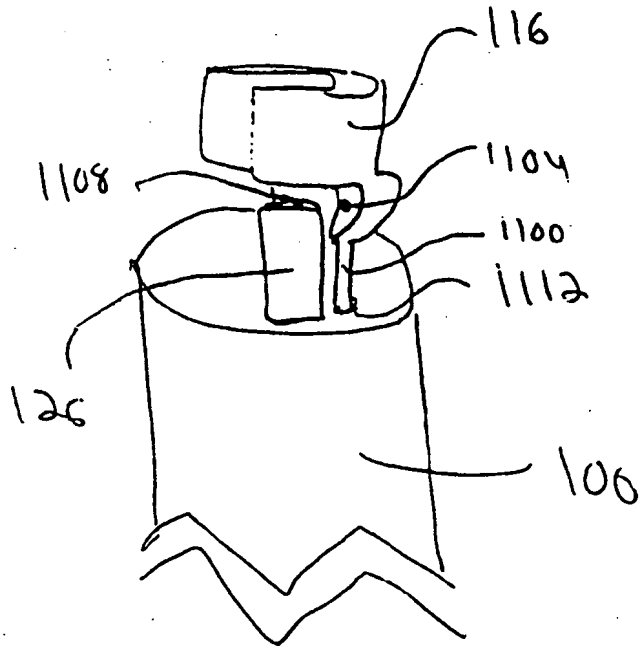

**FOR THE PURPOSES OF INFORMATION ONLY**

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece	ML	Mali	TR	Turkey
BG	Bulgaria	HU	Hungary	MN	Mongolia	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MR	Mauritania	UA	Ukraine
BR	Brazil	IL	Israel	MW	Malawi	UG	Uganda
BY	Belarus	IS	Iceland	MX	Mexico	US	United States of America
CA	Canada	IT	Italy	NE	Niger	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NL	Netherlands	VN	Viet Nam
CG	Congo	KE	Kenya	NO	Norway	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NZ	New Zealand	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	PL	Poland		
CM	Cameroon	KR	Republic of Korea	PT	Portugal		
CN	China	KZ	Kazakhstan	RO	Romania		
CU	Cuba	LC	Saint Lucia	RU	Russian Federation		
CZ	Czech Republic	LI	Liechtenstein	SD	Sudan		
DE	Germany	LK	Sri Lanka	SE	Sweden		
DK	Denmark	LR	Liberia	SG	Singapore		
EE	Estonia						

## CANNULA PROVIDED WITH IRRIGATION MEANS

5

Field of the Invention

This invention relates to a cannula used for endoscopic surgery, and more particularly  
10 to a cannula and method for maintaining a clear visual field for an endoscope housed within  
the cannula.

Cross-Reference to Related Application(s)

The present application is a continuation-in-part application of application serial  
number 09/102,723 filed on June 22, 1998, which prior application is assigned to the same  
15 assignee as the present application.

Background of the Invention

Endoscopic surgery allows a surgeon to perform safe and successful procedures  
because of the surgeon's ability to view the surgical site through the endoscope lens. For some  
surgical procedures, such as dissection, the cannula housing the endoscope has a transparent  
20 blunt dissection tip through which the surgeon views the surgical site. The blunt dissection tip  
protects the endoscope lens from being smeared by blood or fatty tissue present at the surgical  
site, or from being fogged due to the moist subcutaneous environment. However, many  
surgical procedures cannot be performed using a blunt dissection tip. When side branches and  
vessel ends of a vessel must be transected to harvest the vessel, the end of the cannula must be  
25 open to allow the surgical tools to extend from the cannula. When the cannula end is open, the  
endoscope lens is subject to the adverse conditions described above. The surgeon is forced to

repeatedly remove the cannula from the body to clean the endoscope lens. This increases the length and risks of the operation.

Some conventional schemes for cleaning an endoscope lens rely upon an endoscope with a cleaning system built within it. However, having a cleaning system within the  
5 endoscope restricts the angle of incidence at which the cleaning fluid may be propelled toward the lens to almost parallel to the lens. This results in a less effective cleansing action. Also, since the spray is being directed parallel to the lens, the surgeon cannot see the spray source and it is therefore difficult to adjust the direction of the spray. Thus, with these systems, the endoscope must still be removed on occasion for manual cleaning where the proper angle of  
10 incident spray can be obtained manually. Additionally, in procedures using gas insufflation, the gas may dry out a target vessel or other surgical site. In these situations, it is often necessary to irrigate the vessel to prevent the vessel from drying out. However, conventional endoscope washing systems are not capable of providing both endoscope lens cleaning and remote surgical site irrigation. Therefore, a remote endoscopic washing system would be  
15 desirable for more effectively cleansing the endoscope lens during a surgical procedure by allowing the surgeon to control the angle at which cleansing fluid is sprayed as well as allowing the surgeon to use the same apparatus to irrigate the surgical site itself.

#### Summary of the Invention

In accordance with the present invention, a retractor is positioned within a cannula with  
20 a dissection cradle end of the retractor positioned at the distal end of the cannula. The retractor includes a first portion that has an axis approximately parallel to a central axis of the cannula, and a second portion that has an axis which is at an angle with respect to the central axis of the cannula. The dissection cradle is located at the distal end of the second portion of the

retractor. In another embodiment, the retractor includes two legs having substantially parallel axes that selectively protrude from the distal end of the cannula. The protruding legs support the dissection cradle formed in the shape of a partial loop that is positioned in a plane skewed relative to the axes of the legs, with a bottom of the loop directed away from the cannula.

- 5 Thus, in operation, when the surgeon locates a vein and side branch of interest, the surgeon extends the retractor to cradle the vein in the dissection cradle. Once cradled, the retractor may be fully extended, displacing the vein away from the axis of the cannula, causing the side branch to be isolated and exposed to a surgical tool. The surgical tool may then be extended from within the cannula to operate on the isolated and exposed side branch.

- 10 In accordance with one embodiment of the present invention, a remote irrigation system is built into the cannula. In one embodiment, one of the legs which comprise the retractor of the present invention is hollow, and is attached to a spray nozzle disposed in the distal end of the retractor. The proximal end of the hollow leg is attached to a fluid input tube which selectively provides irrigation fluid under pressure for washing the endoscope lens.

- 15 When extended slightly beyond the distal end of the cannula, the spray nozzle is positioned to direct the spray of irrigation fluid at an angle approximately normal to the endoscope lens. This provides for an extremely effective cleaning action, and minimizes the need for removal of the endoscope during surgical procedures for manual cleaning. Additionally, if the surgical site itself requires irrigation, the retractor is extended out of the cannula toward the area
- 20 requiring irrigation, and an irrigation fluid can be sprayed directly on the site. Finally, as the spray is directed back toward the lens, the surgeon can visually adjust the extension of the retractor to accurately direct the spray toward the lens or surgical site.

In a further embodiment, the hollow leg moves within a lumen in the cannula in fluid-resistant sliding engagement, and the fluid input tube is coupled to this lumen. In this embodiment, the maximal outer dimension of a region of the hollow leg is slightly less than a maximal inner dimension of the lumen. The slip-fit, fluid-resistant coupling of the hollow leg within the lumen allows irrigation fluid to be introduced at the proximal end of the lumen by the fluid input tube without significant leakage past the sliding juncture of the hollow leg within the lumen.

In an alternate embodiment, the hollow leg includes a semi-rigid plastic tubing, and fits within an irrigation tube which lines the inside of the lumen. The fluid input tube attaches to the irrigation tube and extends out of the cannula handle for receiving irrigation fluid. The use of flexible, semi-rigid plastic tubes provides fluid seals throughout the irrigation system to minimize leakage. In a third embodiment, the cannula contains a separate irrigation lumen which has a spray nozzle disposed in a fixed position at its distal end. The spray nozzle is positioned within the cannula to allow the proper angle of incidence for the spray to effectively clean the lens. Finally, in another embodiment, the dissection cradle is supported by only one leg, and the lumen which previously held the second leg instead is fitted with a spray nozzle directed toward the endoscope lens. An embodiment is also disclosed in which a nozzle tube situated within a cannula lumen is selectively extensible responsive to the application of hydraulic pressure.

20

#### Brief Description of the Drawings

Figure 1 is a perspective view of a preferred embodiment of cannula 100 showing retractor 112 in an extended position.

Figure 2a is a cut-away side view of retractor 112 and cannula 100.

Figure 2b is a top view of retractor 112.

Figure 3a is a perspective side view of cannula 100 with a saphenous vein positioned within the cradle 116.

Figure 3b is a perspective side view of the distal end 122 of cannula 100 in an embodiment in which an endoscope 126 and a surgical tool 120 are present and partially extended.

Figure 3c is a front view of the distal end 122 of cannula 100 in which the surgical tool 120 and the retractor 116 are partially extended, and an endoscope 126 is present.

Figure 4a is a cut-away top view of cannula 100.

Figure 4b is a cut-away side view of cannula 100.

Figure 5a is a cut-away view of a sliding tube embodiment of cannula 100 in a first position.

Figure 5b is a cut-away view of the sliding tube embodiment of Figure 5a in a second position.

Figure 6a is a cut-away view of an embodiment of cannula 100 having an angling device 140.

Figure 6b is a cut-away side view of the apparatus illustrated in Figure 6a in which the retractor 112 is extended and the angling device 140 is actuated.

Figure 6c is a cut-away side view of the angling device embodiment in which the angling device 140 is in a separate lumen from the retractor 112.

Figure 7a is a cut-away side view of a twistable retractor 112 in a straight position.

Figure 7b is a side view of the retractor 112 of Figure 7a.

Figure 7c is a cut-away side view of twistable retractor 112 in a crossed position.

Figure 7d is a side view of the retractor 112 of Figure 7c.

Figure 8a is a cut-away side view of the handle 104.

Figure 8b is a cut-away side view of an alternate embodiment of handle 104.

Figure 9a is a side view of cradle 116.

5      Figure 9b illustrates a first alternate embodiment of cradle 116.

Figure 9c illustrates multiple views of a second alternate embodiment of cradle 116.

Figure 9d illustrates multiple views of a third alternate embodiment of cradle 116.

Figure 9e illustrates multiple views of a fourth alternate embodiment of cradle 116.

Figure 9f illustrates multiple views of a fifth alternate embodiment of cradle 116.

10      Figure 9g illustrates multiple views of an embodiment of cradle 116 having a spur.

Figure 10a illustrates a top view of an embodiment of the cradle 116 of Figure 9c without a "C" ring.

Figure 10b illustrates a side view of the cradle 116 of Figure 10a.

15      Figure 10c illustrates a top view of the cradle 116 of Figure 9c with the "C" ring attached.

Figure 10d illustrates a side view of the cradle 116 of Figure 10c.

Figure 11a illustrates a perspective side view of a cannula 100 including an irrigation system integrated with the retractor 112.

20      Figure 11b is a cut-away view of a retractor 112 of Figure 11a modified to incorporate the irrigation system.

Figure 11c is a cut-away view of a modified retractor 112 and endoscope 126 situated in a cannula 100.



Figure 11d is an alternate embodiment of the cannula-based irrigation system of Figure 11a.

Figure 12 is a cut-away side view of a multi-tube embodiment of an irrigation system.

Figure 13 is a cut-away side view of an irrigation system including a separate lumen.

5 Figure 14a is a perspective front view of a single leg irrigation system.

Figure 14b is a perspective side view of the single leg irrigation system.

Figure 15 is a flowchart illustrating a method of cleansing an endoscopic lens and irrigating a surgical site in accordance with the present invention.

10 Figure 16a is a cut-away side view of an alternate embodiment of a cannula-based irrigation system in accordance with the present invention.

Figure 16b illustrates the embodiment of Figure 16a when the nozzle 1600 is under hydraulic pressure.

#### Detailed Description of the Preferred Embodiments

Figure 1 illustrates a perspective view of a preferred embodiment of cannula 100 showing retractor 112 in an extended position. Cannula 100 includes an outer housing 102 of bioinert material such as polymed UD that may be approximately 12" to 18" in length. The proximal end of the cannula 100 is disposed in handle 104 that includes a button 106 which is coupled to retractor 112 for controlling the translational movement of retractor 112, as described in more detail below.

20 The distal end of the cannula houses a retractor 112, and optionally an endoscope 126 and a surgical tool 120, described below. Figure 2a illustrates the retractor 112 in more detail. In one embodiment, retractor 112 is formed of resilient wire which has a smooth bend intermediate to a first portion 110 and a second portion 114 of the retractor. The retractor 112

is described as having two portions for ease of description, although the retractor 112 may be formed as an integrated structure. However, retractor 112 may also be manufactured from two separate portions 110, 114 that are coupled together. The first portion 110 of the retractor 112 is positioned within the cannula 100 with the axis 111 of the first portion 110 approximately  
5 parallel to the axis 101 of the cannula 100. The second portion 114 is positioned to bend away from the central axis 101 of the cannula. The angle 117 of displacement between the axis 115 of the second portion and the central axis 101 of cannula 100 may be any angle from zero to 180 degrees. The second portion 114 includes a dissection cradle 116 at the distal end of the second portion 114. The retractor 112 may be formed of bioinert material such as stainless  
10 steel, or a polymer such as nylon or polyetherimide, or other appropriately strong and resilient plastic. In one embodiment, the retractor 112 includes a coating for lubrication, insulation, and low visual glare using, for example, parylene or nylon 11.

Figure 2b illustrates the retractor 112 formed with two legs. The legs 141, 142 of the retractor 112 at the distal end form the dissection cradle 116 in a loop or "U" shape, as shown  
15 in Figure 2a. The top portion 144 of the U-shaped bend is preferably flattened to provide additional surface area for atraumatically supporting a vein 118 or vessel of interest. The side arches 128 of the dissection cradle 116 are used for skeletonizing or dissecting the vein from the surrounding tissues, as well as acting as walls to keep the vessel captured within the arch. The several embodiments of dissection cradle 116 are described in more detail below.

20 Figure 3a illustrates a perspective view of the cannula 100 in accordance with the present invention with the retractor fully extended, holding a saphenouss vein 118, and also illustrates an external surgical tool 120 disposed adjacent the cannula 100 for performing a surgical operation, for example, severing a tributary or side branch of the vein 118. The vein

is positioned within the side arches 128 of the cradle 116. The dissection cradle 116 may be used to cradle a vein, vessel, tissue or organ of interest, and surgical tool 120 may be any surgical tool suitable for performing a surgical procedure near the dissection cradle 116.

Figure 3b illustrates a perspective view of cannula 100 in an embodiment in which the surgical tool 120 is positioned within the cannula 100, and an endoscope 126 is present. In this embodiment, cradle 116 preferably overlays the endoscope 126 with sufficient clearance to facilitate relative movements thereof. However, the endoscope may also be located adjacent the surgical tool 120. In one embodiment, endoscope 126 is positioned with cannula 100 to allow a clear field of view upon extension of the retractor 112. Surgical tool 120 is illustrated as cauterizing scissors, used to sever a tributary or side branch of a saphenous vein 118. In this embodiment, surgical tool 120 is maximally displaced from the cradle 116 at the cannula end 122. More specifically, as shown in Figure 3c, the "U"-shaped loop 129 of the cradle 116 is closest to the surgical tool 120. This ensures that a vein 118 or other tissue of interest is retracted away from the surgical tool 120 to facilitate manipulating the surgical tool 120 relative to the side branch or other tissue.

Figure 4a is a cut-away top view of cannula 100. The retractor 112 is slidably positioned within minor lumens 113 along the length of the cannula 100 within close tolerances in order to position the retractor 112 stably within the cannula 100. For example, in one embodiment retractor legs 141, 142 are approximately .045 inches in diameter and the lumens 113 encasing the legs 141, 142 are approximately .080 inches in diameter, as friction between the legs of the retractor 112 and the lumens 113 holds the retractor stably within the cannula. This configuration restricts rotational movement of the retractor to provide more stable retraction as compared with conventional retractors. The legs 141, 142 of the retractor

112 are formed of flexible, resilient material and are retained within the lumen 113 in substantially straight or flat orientation, but may return to a material bend or curve, as illustrated in Figure 5a, as the retractor 112 is extended from the distal end of the cannula 100.

The leg 141 of the retractor 112 passes through a sliding gas or fluid seal 130 at the proximal end of the lumen 113. The leg 141 of the retractor 112 passes out of the cannula 100 and into handle 104 for attachment to a slider button 106 for facilitating translational movement of the retractor 112 from the proximal or handle end of the cannula 100. However, other types of control devices such as knobs, grips, finger pads, and the like may be linked in conventional ways to the retractor 112 in order to manually control the translational movement of retractor 112. In one configuration, the proximal end of leg 141 is bent relative to the axis of the cannula, and the button 106 is attached to the bent position of the leg 141 to facilitate moving the button 106 and the retractor 112 translationally under manual control. The button 106 preferably includes lateral grooves to prevent finger or thumb slippage during sliding manipulation of the retractor 112.

Thus, in the operation of a preferred embodiment, a user actuates the slider button 106 to extend retractor 112 out of the lumen 113 at the distal end of the cannula 100. In one embodiment, the resilient retractor 112 is formed in a smooth bend, as shown in Figure 2a, and gradually deflects away from the central axis 101 of the cannula 100 as the retractor is extended. Upon encountering the target vessel or tissue of interest, the vessel is restrained in the cradle 116, and a lateral resilient force is exerted on the target vessel in a direction away from the cannula. The vessel is thus pushed away from the axis of the cannula 100, isolating it from surrounding tissue or adjacent vessels such as tributaries or side branches. As a tributary is thus isolated, a surgical tool 120 such as cauterizing scissors may be safely employed to

operate on the tributary without harming the saphenous vein 118. When retracted into the cannula 100, the retractor 112 is again resiliently straightened or flattened.

In an alternate embodiment as illustrated in Figures 5a and 5b, a sliding tube 132 is added to provide operational versatility to cannula 100. In a first position, the sliding tube 132 is retracted and the retractor 112 protrudes from the distal end at an angle with respect to the central axis 101 of the cannula 100. In a second position, the sliding tube 132 is extended out, temporarily straightening the retractor 112. As illustrated in Figure 5a, a sliding tube 132, in a first position encases the retractor 112 up to the point at which the retractor 112 curves away from the central axis 101 of the cannula thus allowing the retractor 112 to displace and isolate a target vessel. The proximal end of the sliding tube 132 is linked to button 107 for translationally moving retractor 112 as well as actuating the sliding tube 132. In one embodiment, as illustrated in Figure 5a, the sliding tube 132 is in a first position with the button 107 in an upright position. A spring 134 is coupled between a support structure 135 and the proximal end 137 of the sliding tube 132. In the first position of sliding tube 132, the spring 134 is extended fully and exerts little or no force on the sliding tube 132. Of course, sliding tube 132 may be manually manipulated without linkage to a button 107.

To extend the sliding tube 100, button 107 is pushed down. As illustrated in Figure 5b, the button 107 has a cam surface 136 which pushes on the proximal end 137 of the sliding tube 132 as the button 107 is pressed. The sliding tube 132 is pushed forward, overcoming the resilient force of spring 134, to encase the retractor 112 and decrease angle 117 between the distal end of the retractor 112 and the central axis 101 of the cannula 100. Upon releasing the button 107, the spring force urges the proximal end 137 of the sliding tube 132 back toward the first position against button 107. The sliding tube 132 is formed of material having

sufficient strength to force the retractor 112 to straighten out the angle 117, and the retractor 112 is formed of resilient material having a sufficient flexibility to straighten out the angle 117 in response to a tube 132 being slid over the retractor 112, but having sufficient rigidity to cradle and dissect a target vessel. Resiliency of the retractor 112 ensures return to the  
5 downwardly-curved shape after being released from tube 132. Thus, in accordance with this embodiment, a user may employ the curved retractor for certain applications and employ the straightened form for other applications. A manual actuator may be configured in other ways than button 107 to extend the sliding tube 132 in response, for example, to being pulled up instead of pushed down.

10 Another embodiment employs a retractor 112 which has a naturally straight shape. As illustrated in Figures 6a and 6b, an angling device 140 is disposed between the distal end of the retractor 112 and the proximal end of the cannula. The angling device 140 may be positioned within the same lumens 113 as the retractor 112 and preferably may comprise two wires coupled to points below the cradle 116 of the retractor 112 substantially in parallel  
15 positions on each of the legs 141, 142.

Upon extending the retractor 112 using button 106, the angling device 140 is extended with the retractor 112. The angling device 140 is coupled to a handle 145 at the proximal end of the cannula 100 to facilitate establishing an angle in the retractor 112 by pulling with a backward force on the angling device 140. As illustrated in Figure 6b, after the retractor 112  
20 is extended, the angling device 140 is actuated and a bend is created in the retractor 112 as the backward force exerted on the distal end of the retractor is exerted against the relatively fixed position of the retractor legs 141, 142 disposed within the lumens 113. As shown in Figure 6c, the angling device 140 may also be located in a separate lumen 202 from the retractor 112 with

part of the angling device 140 positioned outside of the cannula 100 when the retractor 112 is in the retracted position.

Figure 7a illustrates another embodiment of cannula 100 in which the retractor 112 is pre-formed with one leg 141 of the retractor 112 bent at an angle at its proximal end skewed to the axis of the distal end of the other leg 142. The bent portion of the leg 141 may be linked to a sliding knob 147 for convenient manual manipulation of this embodiment of the invention. Upon sliding the knob 147, the leg 142 coupled to knob 147 is twisted rotationally. The two legs 141, 142 of retractor 112 are coupled together via cradle 116. The axis of the second portion of the retractor 112 in the first position is at a first angle 117 to the axis of the cannula 100, as shown in Figure 7b. As knob 147 is moved, leg 141 is rotated and crosses under leg 142, as shown in Figure 7c. This causes cradle 116 to flip 180 degrees and bends the retractor 112 at a second angle 119, as shown in Figure 7d. Thus, if a vessel is disposed on one side of cradle 116 or cannula 100 while the retractor 112 is in the first position, then upon rotating the knob 147, the vessel is transported to the other side of the cannula 100. This allows the user to isolate the vessel by simply actuating knob 147.

Figure 8a illustrates a cut-away side view of button 106 on the handle 104 of cannula 100, with an endoscope 126 positioned within cannula 100. As mentioned above, button 106 is coupled to one leg 141 of the proximal end of retractor 112. Sliding the button 106 in groove 146 translationally moves the retractor 112. Groove 146 is preferably minimally wider than the shaft of button 106 to minimize excessive horizontal movement of button 106 while still allowing smooth translational movement of button 106. As illustrated in Figure 8b, the button 106 may include locking or ratcheting teeth 152 to give tactile feedback of its location, and to positively retain the button and the associated leg 141 in an extended or retracted

position. Several mating teeth 148 are located underneath groove 146, and a spring member 150 is attached to button 106 to exert pressure against the base of groove 146, to engage mating teeth 148, 152. When a force is applied on the top of button 106, the interlocking sets of teeth are disengaged and button 106 can move freely. Upon achieving the desired extension or retraction of the leg 141, button 106 is released and is retained place by the engaged teeth 148, 152.

Figure 9a illustrates a top view of cradle 116 in an embodiment in which the cradle 116 is formed by two legs 141, 142 of retractor 112. The distal end of the legs form "U"-shaped side guides. The top 144 of the distal portion of the "U" is preferably flattened. This provides atraumatic support for the target vessel retained within cradle 116. Additionally, by minimizing the thickness of distal portion 144, contact with other devices in close proximity with retractor 112 is minimized.

The cradle 116 may have other effective shapes, for example, as illustrated in Figure 9b in which a "C" ring element is attached to legs of the cradle 116. The "C" ring may have a small hole 200 in one side with an axis approximately parallel to the axis of the retractor 112. This hole 200 is used to hold suture or other ligating materials, and may also be used as a knot pusher. As shown in Figures 10a and 10b, in an alternate embodiment of the embodiment of Figure 9b, the retractor 112 is formed and flattened and a "C"-shaped ring is coupled to the retractor 112 by, for example, gluing or molding the "C" ring to the distal end of the retractor 112, as shown in Figure 10c and 10d.

Referring back to Figures 9c, 9d, and 9e, the side guides of the cradle may include a loop 129 in a "V" shape, an arced "U" shape, or a semi-circular shape. In one embodiment, as illustrated in Figure 9f, the retractor 112 has only one leg 141, and the cradle 116 is formed by



the leg 141. A stopper 160 is coupled to the end of the leg 141 to serve as a guide to retain the target vessel, and add a blunt surface to the end of the wire, for example, for pushing and probing tissue. Figure 9g illustrates a retractor 112 having a spur 204 formed in one or both legs 141, 142 for allowing the retractor 112 to be used for dissection. Sinusoidal, half-  
5 sinusoidal, and other geometric configurations may be used equally effectively as the shape of loop 129 in accordance with the present invention.

Figure 11a illustrates a perspective side view of a cannula 100 and an irrigation effector 1150 for cleaning an endoscope lens 1108 and wetting a surgical site. In the embodiment of Figure 11a, the irrigation effector is retractor 112. As described above, the retractor 112  
10 extends distal to the tip of the cannula 100 responsive to activation of a control button 106. In one embodiment, two supporting members 1100, 141 attach to the dissection cradle 116 and allow it to extend and retract. As shown in Figure 11b, one supporter or leg 1100 is hollow, functioning as a lumen to carry irrigation fluid for cleaning an endoscope lens 1108 (shown in Figure 11c). An irrigation nozzle 1104 is disposed on the cradle 116 or on the distal portion of  
15 the hollow leg 1100 and is configured to spray irrigation fluid at the endoscopic lens 1108. The irrigation fluid is received from a fluid source which conducts the fluid under pressure to the leg 1100. When the retractor 116 is slightly extended out of the distal end of the cannula 100, the irrigation nozzle 1104 is directed toward the lens 1108 of the endoscope 126 at an angle approximately normal to the endoscope lens 1108, allowing a spray of irrigation fluid to  
20 contact the surface of the lens 1108 and clean the lens 1108 effectively. Additionally, as the spray is directed back toward the endoscope 126, the surgeon is able to view the source of the spray through the endoscope 126, and is able to adjust the angle of incidence by adjusting the extension of the retractor 112. Thus, by having the endoscopic washing system built into the

cannula 100 and into the sliding retractor 112, a more effective cleaning system is provided than what is provided by systems which are built into the endoscope itself.

If the surgical site requires irrigation, the dissection cradle 116 is extended out of the cannula 100, as shown in Figure 11a, toward the area requiring irrigation. Upon reaching the site under endoscopic visualization, the surgeon can direct a spray of irrigation fluid toward the site. Again, if the site is not properly irrigated, the surgeon can adjust the positioning of the retractor 112 until the spray has contacted the surgical site. Thus, the irrigation system of the present invention can both wash the endoscope lens 1108 and irrigate a remote surgical site.

As shown in Figure 11c, the hollow leg 1100 is situated within a lumen 1112 in the cannula body 100. An extension tube (not shown) is connected to the proximal end of the lumen 1112 to provide a source of irrigation fluid under pressure, for example, via a Luer lock syringe fitting. The syringe is used to selectively inject fluid under pressure into the lumen 1112 upon a determination that the endoscope lens 1108 requires cleansing. The hollow leg 1100 may extend only a fraction of the length of the lumen 1112 within the cannula body 100 prior to coupling to irrigation fluid under pressure. However, the hollow leg 1100 should be of sufficient length to extend the cradle 116 out to its proper working distance. To minimize leakage of irrigation fluid, the hollow leg 1100 has an outer diameter that slip fits within the inner diameter of the cannula body lumen 1112. Alternatively, as shown in Figure 11d, the hollow leg 1104 has an outer diameter smaller than the inner diameter of the cannula body lumen 1112, but has a proximal end 1120 that flares out to a slip fit within the cannula body lumen 1112. These relative dimensions allow irrigation fluid to be dispensed through the

cannula body lumen 1112, into the hollow leg 1100 and out the irrigation nozzle 1104 without significant leakage past the hollow leg 1100.

Figure 11d illustrates an embodiment of the single-leg irrigation system in which a wire 141 is present within the hollow leg 1100 in lumen 113. The presence of wire 141 provides support and rigidity to the retractor 112 while retaining the ability of the hollow leg 1100 to be used to conduct irrigation fluid to the irrigation nozzle 1104.

Figure 12 is a cut-away side view of a multi-tube embodiment of a cannula-based irrigation system. In this embodiment, the hollow leg 1200 includes a semi-rigid flexible tube or the like, and extends approximately one quarter to one third of the length of the cannula body 100 within a second irrigation tube 1204 inside of the cannula body lumen 1112. A fluid input tube 1208 of flexible plastic attaches to the proximal end of the irrigation tube 1204 and extends out of the cannula handle 104. The proximal end of the fluid input tube 1208 may include a valved Luer lock fitting 1212 for connection to a source of irrigation fluid such as provided by a syringe by selective applications of pressure. The first tube 1200 is slidable within the irrigation tube 1204 to form an adequate sliding fluid seal between the moving parts.

Figure 13 is a cut-away side view of a separate lumen irrigation system. In this embodiment, the cannula 100 contains a separate irrigation lumen in the cannula body. The lumen ends in a spray nozzle 1300 on the distal tip of the cannula 100. The tip of the nozzle 1300 is approximately parallel to the lens 1108. Cleansing is accomplished by applying spraying irrigation fluid across the lens 1108 to wash the lens 1108. The irrigation fluid is supplied to the irrigation lumen by a fluid input tube 1208 as described above in Figure 12, and the proximal end of the fluid tube 1208 may be attached to a syringe as a source of the

irrigation fluid under selective pressurization. The syringe may be removeably attached to the cannula handle 104 to prevent the syringe from moving or dangling from the handle 104, and obtruding on manipulation of the cannula 100 during vessel harvesting.

Figure 14a is a perspective front view of a single leg irrigation system and shows the distal end of the cannula 100 housing the cradle 116 and the endoscope 126. In this embodiment, the dissection cradle 116 is supported by one leg 141 (shown in Figure 11b) within a first lumen 1408 within the cannula body 100, and a cannula body lumen 1412 not occupied by the second leg of the cradle 116, as in embodiments previously described, is fitted with a nozzle 1400 which sprays the endoscope lens 1108. The spray nozzle 1400 is directed at an angle at which the endoscope lens 1108 can be sprayed directly and effectively for cleaning. Figure 14b is a perspective side view of the single leg irrigation system and shows the distal end of the cannula 100 and the location of the spray nozzle 1400.

Figure 15 is a flowchart illustrating a method for washing an endoscopic lens 1108 and remote surgical site in accordance with the present invention. First, skin is incised 1500 at an area near a target vessel. Next, the device is advanced 1504 under endoscopic visualization toward the surgical site. If the surgeon determines 1506 that the surgical site has been reached, then the surgeon determines 1520 whether the surgical site requires irrigation. If the surgical site requires irrigation, the surgeon extends 1524 the retractor 112 toward the surgical site and activates 1528 the irrigation system to wet the surgical site. The surgeon determines 1532 whether the site is sufficiently wet by viewing the site through the endoscope 126. If the site is sufficiently wet, the process ends. If the site requires more irrigation, the surgeon positions 1536 the retractor 112 under endoscopic visualization to direct the spray more accurately at the surgical site.

If the surgical site has not been reached, the surgeon determines 1508 whether the lens 1108 is clean. In response to the lens 1108 becoming obscured with blood, fatty tissue, or the like, the irrigation system is activated 1512 in situ to wash the lens 1108. In one embodiment as described above, the retractor 112 is extended until the angle of the spray is approximately  
5 normal to the surface of the endoscopic lens 1108, and therefore effectively washes the lens 1108. Next, the surgeon determines 1514 whether the lens 1108 has been cleaned satisfactorily. If not, the retractor and thereby the irrigation nozzle 1104 is selectively positioned 1516 via extension or retraction of the retractor 112 under endoscopic visualization to direct the spray toward the lens 1108 at a more effective angle. The surgeon can continue to  
10 reposition the retractor 112 until the spray nozzle is directed at an effective angle toward the lens 1108.

Figure 16a shows a cut-away side view of another embodiment of a cannula-based irrigation system. In this embodiment, a nozzle tube 1600 is extendable from within a lumen 113 in the cannula 100. The proximal end of the nozzle tube 1600 is attached to a distal end of  
15 a tension spring 1604, whose proximal end is stably attached on the side of the lumen 113 or at the proximal end of the cannula 100. The tension spring 1604 biases the nozzle tube 1600 in a retracted state. Upon exposure to hydraulic water pressure, as shown in Figure 16b, the liquid pushes the nozzle tube 1600 out of the lumen to a point slightly beyond the endoscope lens 1108. The liquid flows inside the nozzle tube 1600 and exits out the spray hole 1608, spraying  
20 irrigation fluid back towards the endoscope lens 1108.

Thus, the irrigation systems described above provide an effective method of cleaning an endoscope lens 1108 without requiring the removal of the endoscope from a surgical site. Additionally, the washing system described above is more effective due to the use of a spray

nozzle external to the endoscope, which allows the angle of spray to be directly projected against the endoscope lens 1108. In an embodiment in which the irrigation nozzle 1104 is disposed on the cradle 116 or on the hollow leg 1100, a surgeon can visually adjust the angle of incidence of the spray, and can also irrigate a surgical site by adjusting the extension of the

5 retractor 112 out of the cannula 100.

CLAIMS

What is claimed is:

1. A surgical apparatus for generating an irrigating spray comprising:  
an elongated cannula having an axis between distal and proximal ends, and  
5 an irrigation effector, slidably supported on at least one hollow supporter  
relative to the cannula for translational movement substantially aligned  
with the axis of the cannula, and including an irrigation nozzle disposed  
near the distal end of the hollow supporter, the hollow supporter  
conducting irrigation fluid to the irrigation nozzle.
- 10 2. The apparatus of claim 1 wherein the irrigation nozzle is disposed in a side of the  
hollow supporter near the distal end thereof.
3. The apparatus of claim 1 wherein the hollow supporter is disposed within an irrigation  
conduit in the cannula and a proximal end of the irrigation conduit includes a fluid inlet.
4. The apparatus of claim 3 wherein the hollow supporter is semi-rigid plastic tubing that  
15 is slip-fitted within the irrigation conduit near the distal end of the cannula.
5. The apparatus of claim 1 wherein the irrigation effector is a retractor.
6. The apparatus of claim 5 wherein the cannula further comprises a retractor lumen  
therein for supporting the hollow supporter in slip-fitting relationship with the retractor lumen.
7. The apparatus of claim 5 wherein the retractor further comprises a dissection cradle,  
20 disposed at the distal end of the retractor, and the irrigation nozzle is disposed in the dissection

cradle that includes a conduit therein in fluid communication between the hollow supporter and the nozzle.

8. The apparatus of claim 1 further comprising a tension spring, having a distal end attached to the distal end of the hollow supporter, for allowing the extension of the distal end of the hollow supporter beyond the distal end of the cannula responsive to an application of pressure, and retaining the hollow supporter in a retracted position otherwise.

9. A surgical apparatus for cleansing an endoscope lens that can be positioned within a surgical site, the apparatus comprising:

an elongated cannula having an axis between distal and proximal ends, the

10 cannula comprising:

an endoscope lumen, for housing an endoscope therein; and

an irrigation lumen, having a distal end and a proximal end, and having

a spray nozzle disposed at the distal end, for conducting

irrigation fluid to an endoscope housed in the endoscope lumen;

15 and

a fluid inlet near the proximal end of the irrigation lumen for conducting fluid to the spray nozzle via the irrigation lumen.

10. The apparatus of claim 9 in which the spray nozzle is positioned at a point distal to the endoscopic lens, and is directed toward the endoscopic lens.

20 11. The apparatus of claim 9 wherein the cannula includes an additional lumen for slidably supporting therein a supporter for a retractor disposed at a distal end of the supporter.



12. A method for cleansing an endoscope lens at a distal end of an elongated cannula that slidably supports a retractor for selecting extension from the distal end of the cannula and that includes an irrigation system, comprising the steps of:

- incising skin at an area near a target vessel;
- 5       advancing the cannula through the incision towards a target site under  
          endoscopic visualization through the endoscope lens at the distal end of  
          the cannula;
- selectively extending the retractor to position the spray nozzle thereon to wash  
          the lens of the endoscope. and
- 10       selectively activating the irrigation system for washing the endoscope lens.

13. A method of irrigating a remote surgical site using an elongated cannula that slidably supports a retractor for selecting extension from the distal end of the cannula and that includes an irrigation system, comprising the steps of:

- incising skin at an area near a target vessel;
- 15       advancing a cannula through the incision towards the surgical site under  
          endoscopic visualization;
- responsive to the surgical site requiring irrigation, selectively extending the  
          retractor toward the surgical site; and
- activating the irrigation system for wetting the surgical site.

1/15






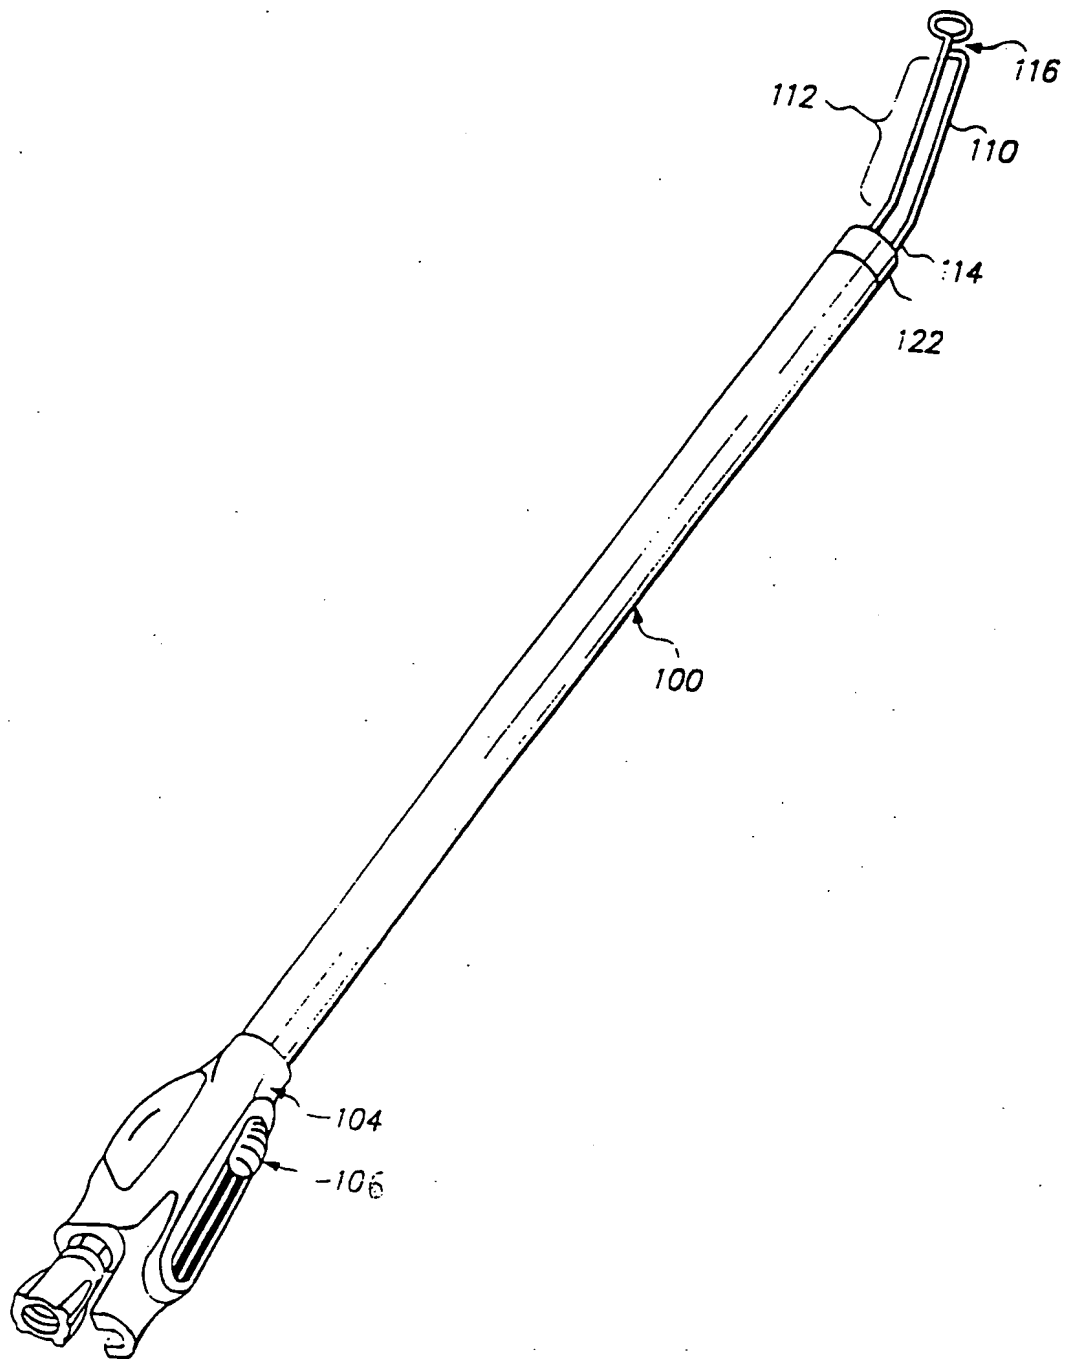


FIG. 1

2/15

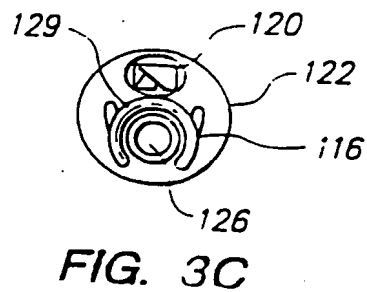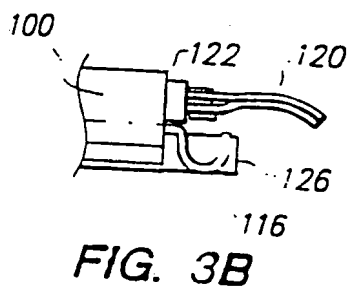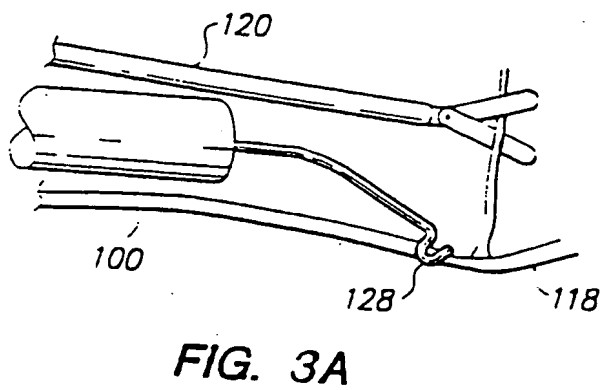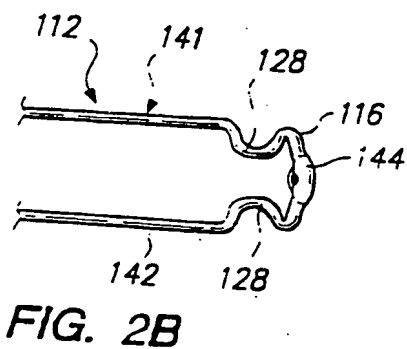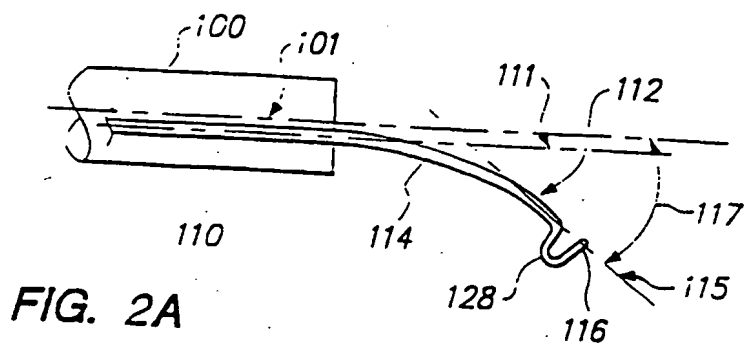

3/15

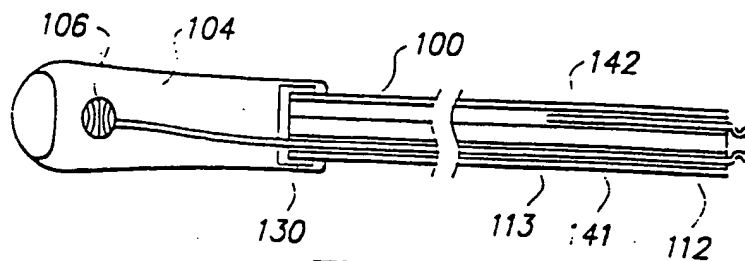


FIG. 4A

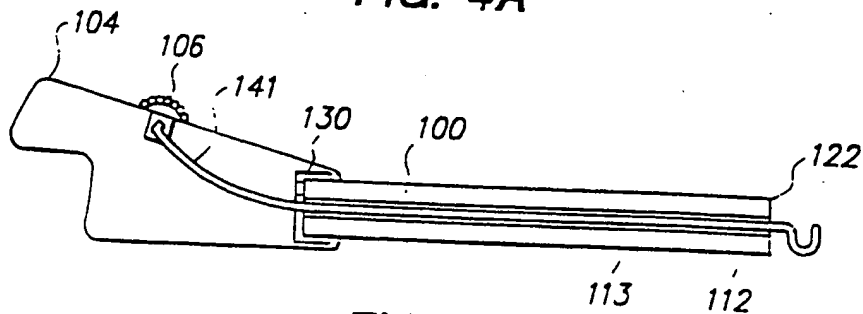


FIG. 4B

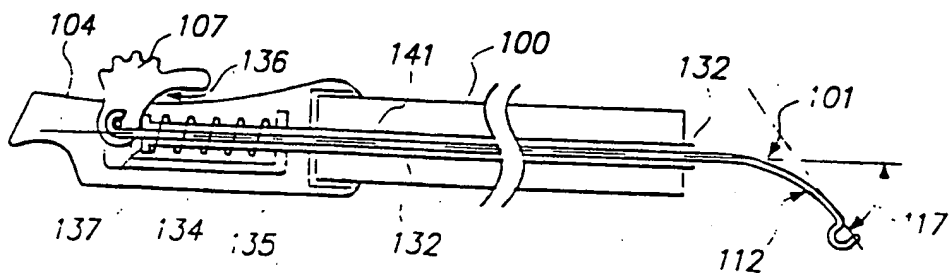


FIG. 5A

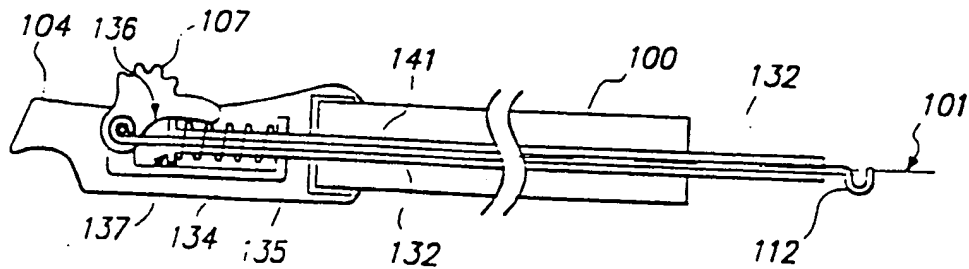


FIG. 5B

4/15

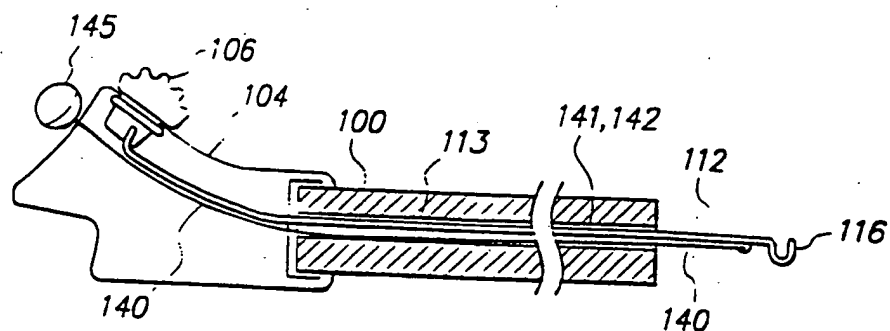


FIG. 6A

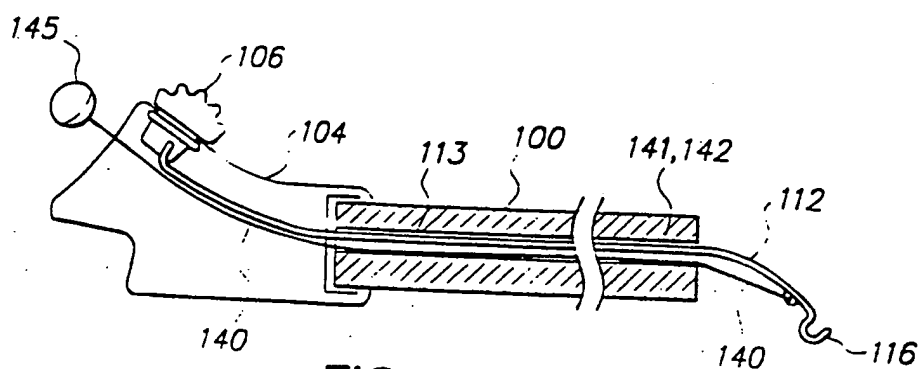


FIG. 6B

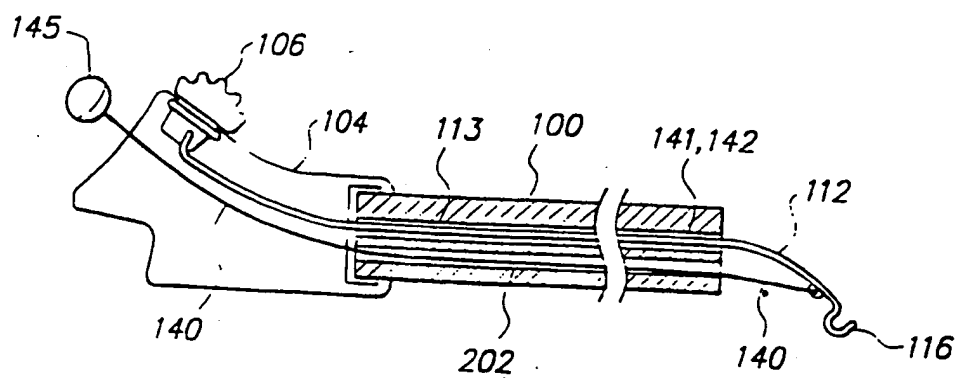


FIG. 6C

5/15

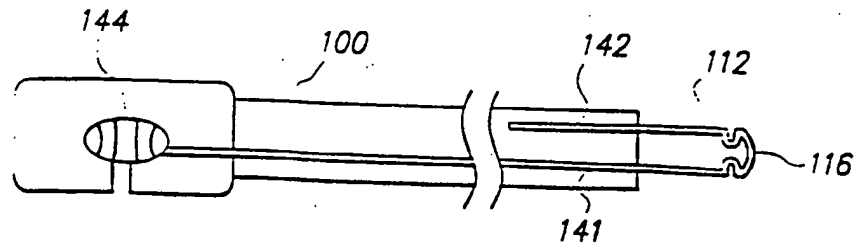


FIG. 7A

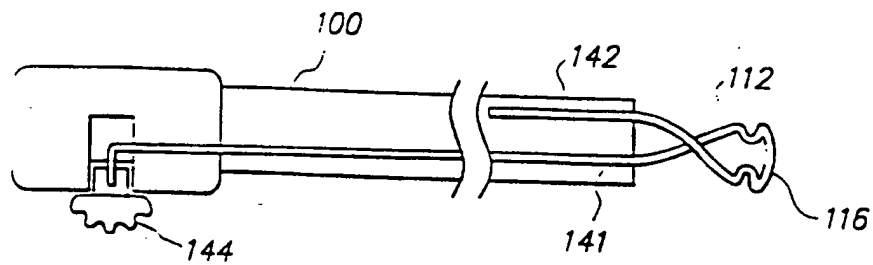


FIG. 7C

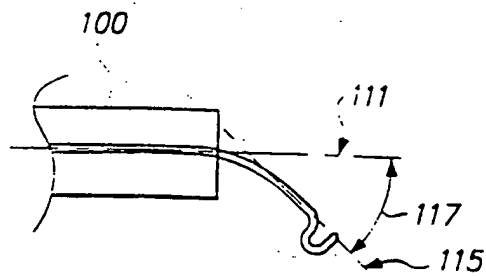


FIG. 7B

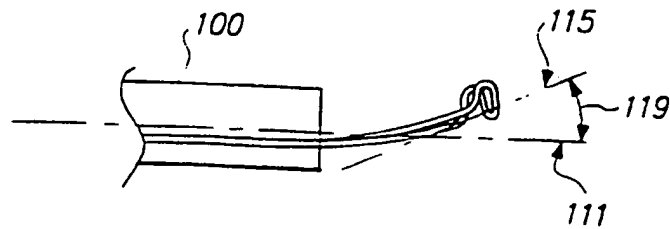


FIG. 7D

6/15

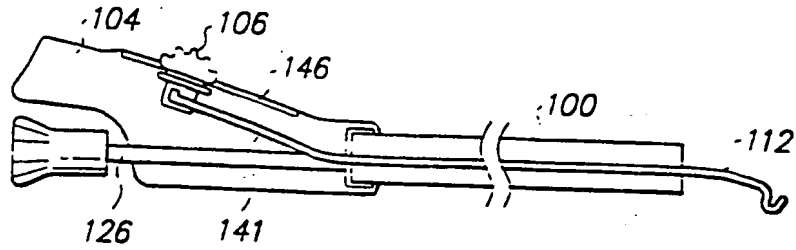


FIG. 8A

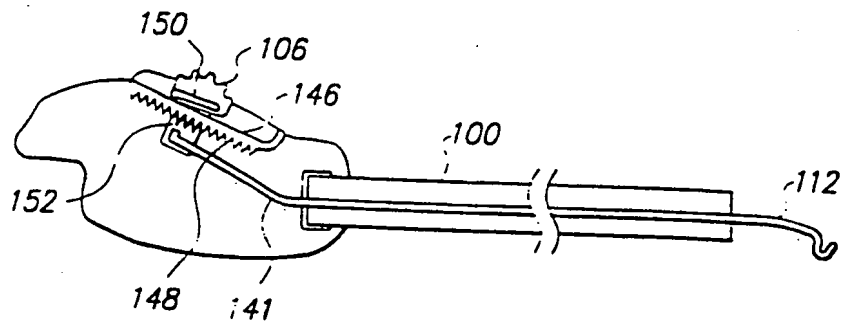


FIG. 8B

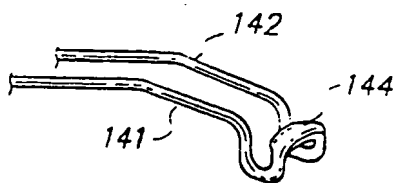


FIG. 9A




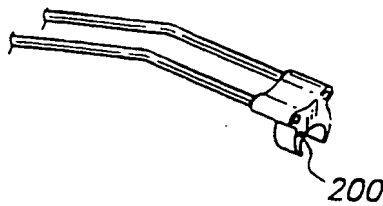


FIG. 9B

7/15

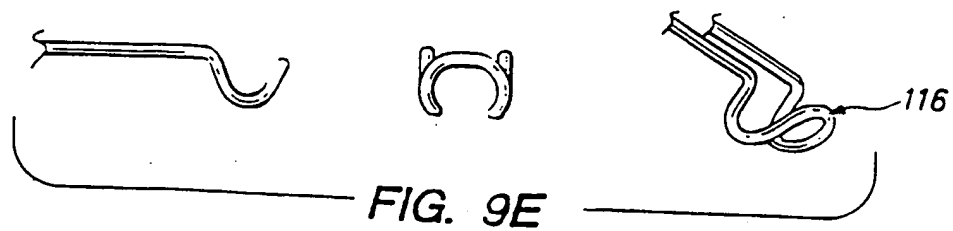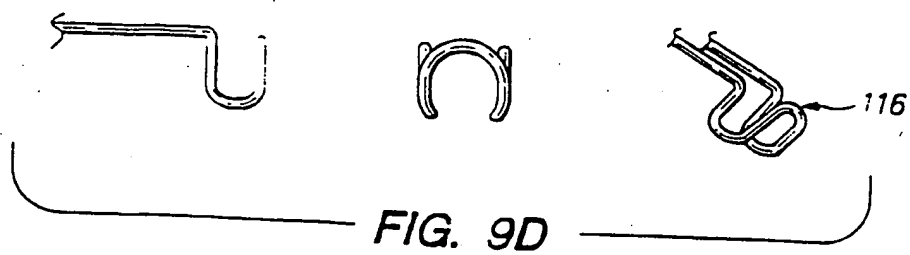

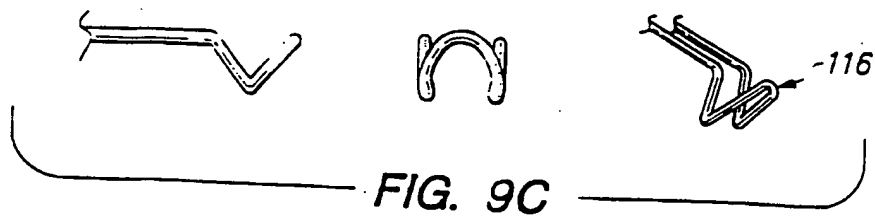

8/15

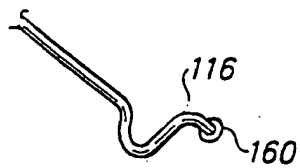


FIG. 9F

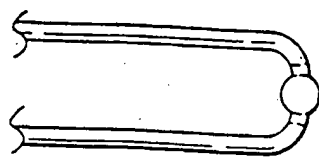
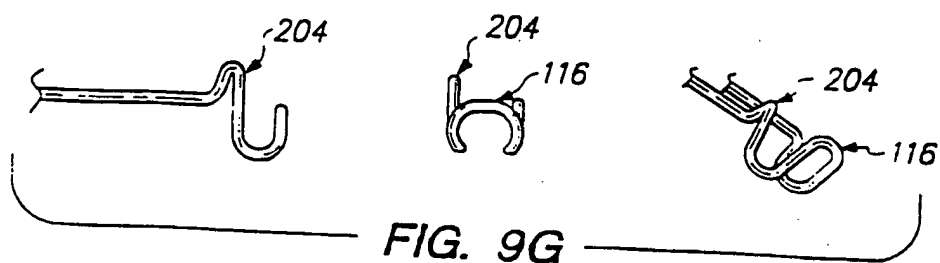


FIG. 10A



FIG. 10B

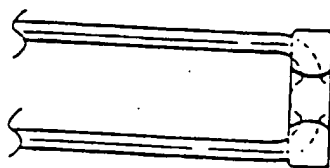


FIG. 10C





FIG. 10D

9/15

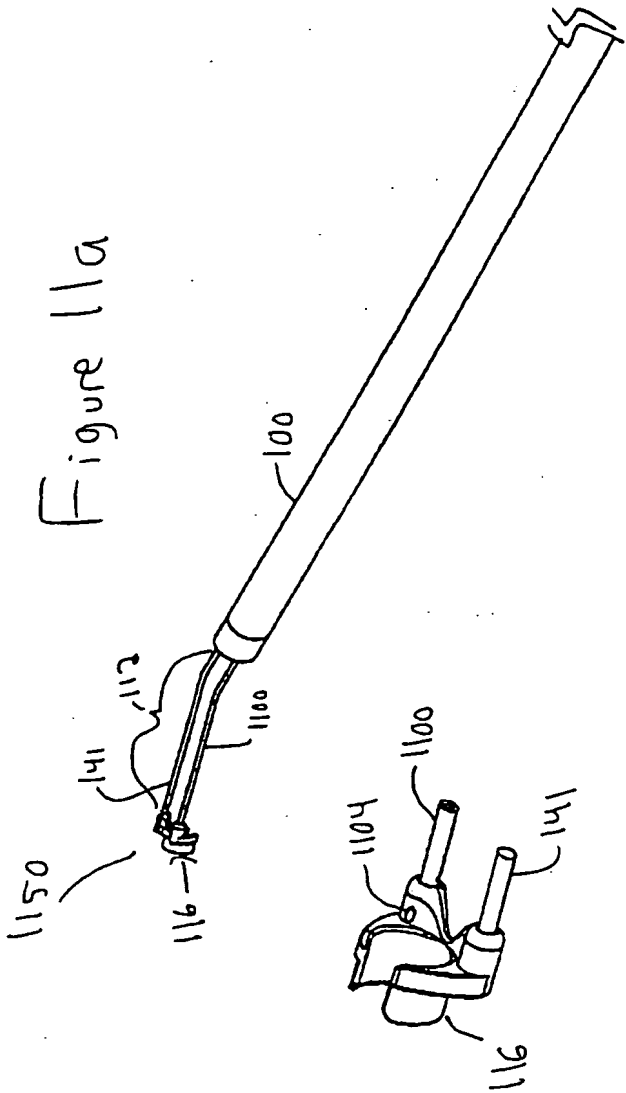

10/15

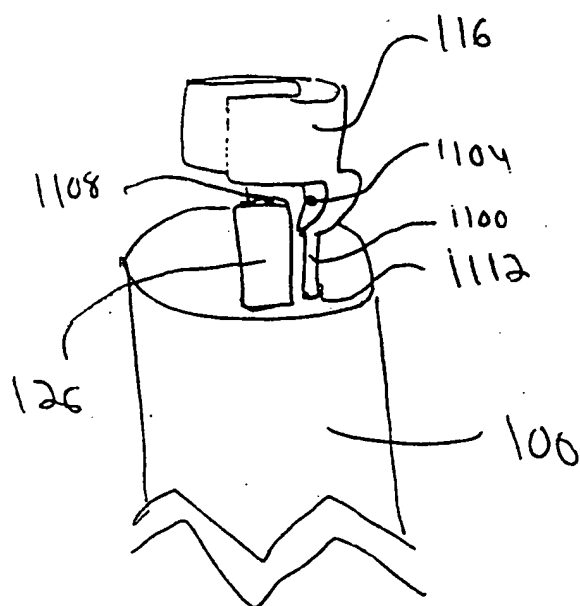


Figure 11c

11/15

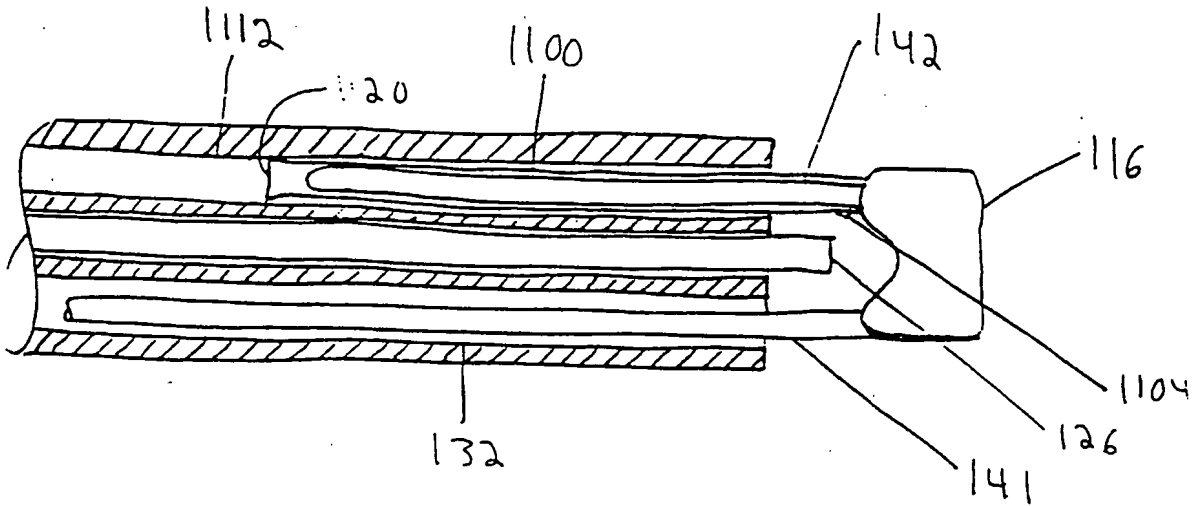


Figure 11d

12/15

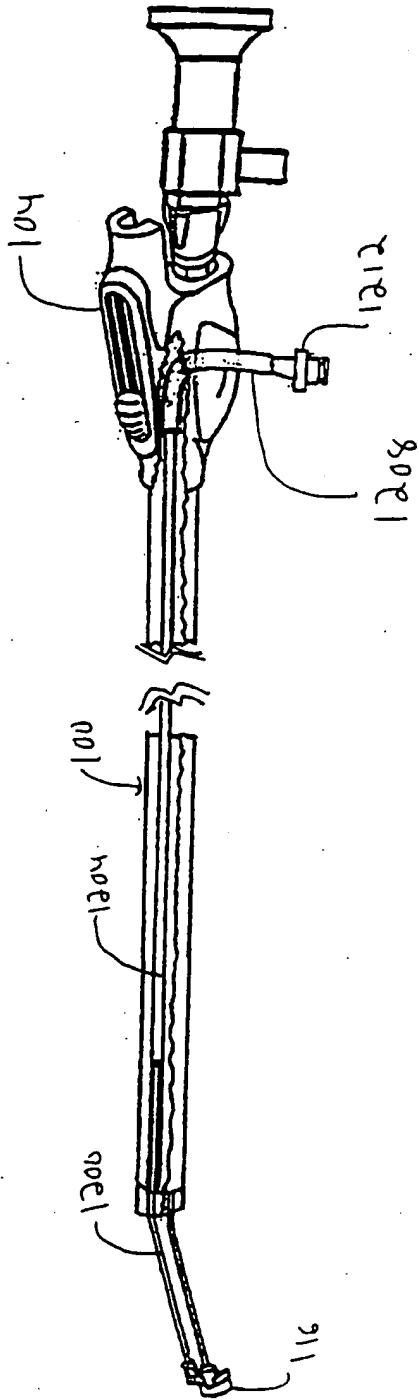


Figure 12

13/15

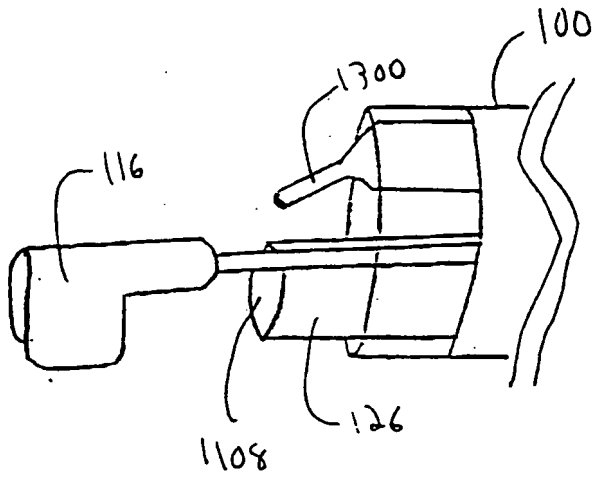


Figure 13

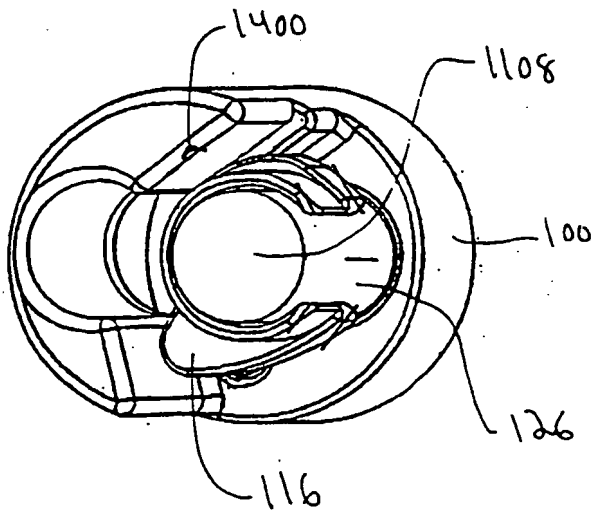


Figure 14a

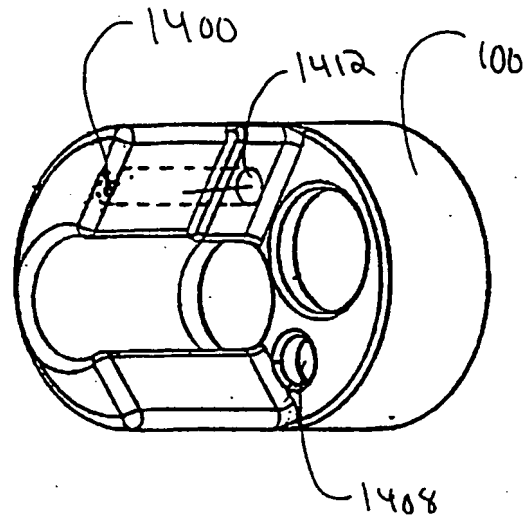


Figure 14b

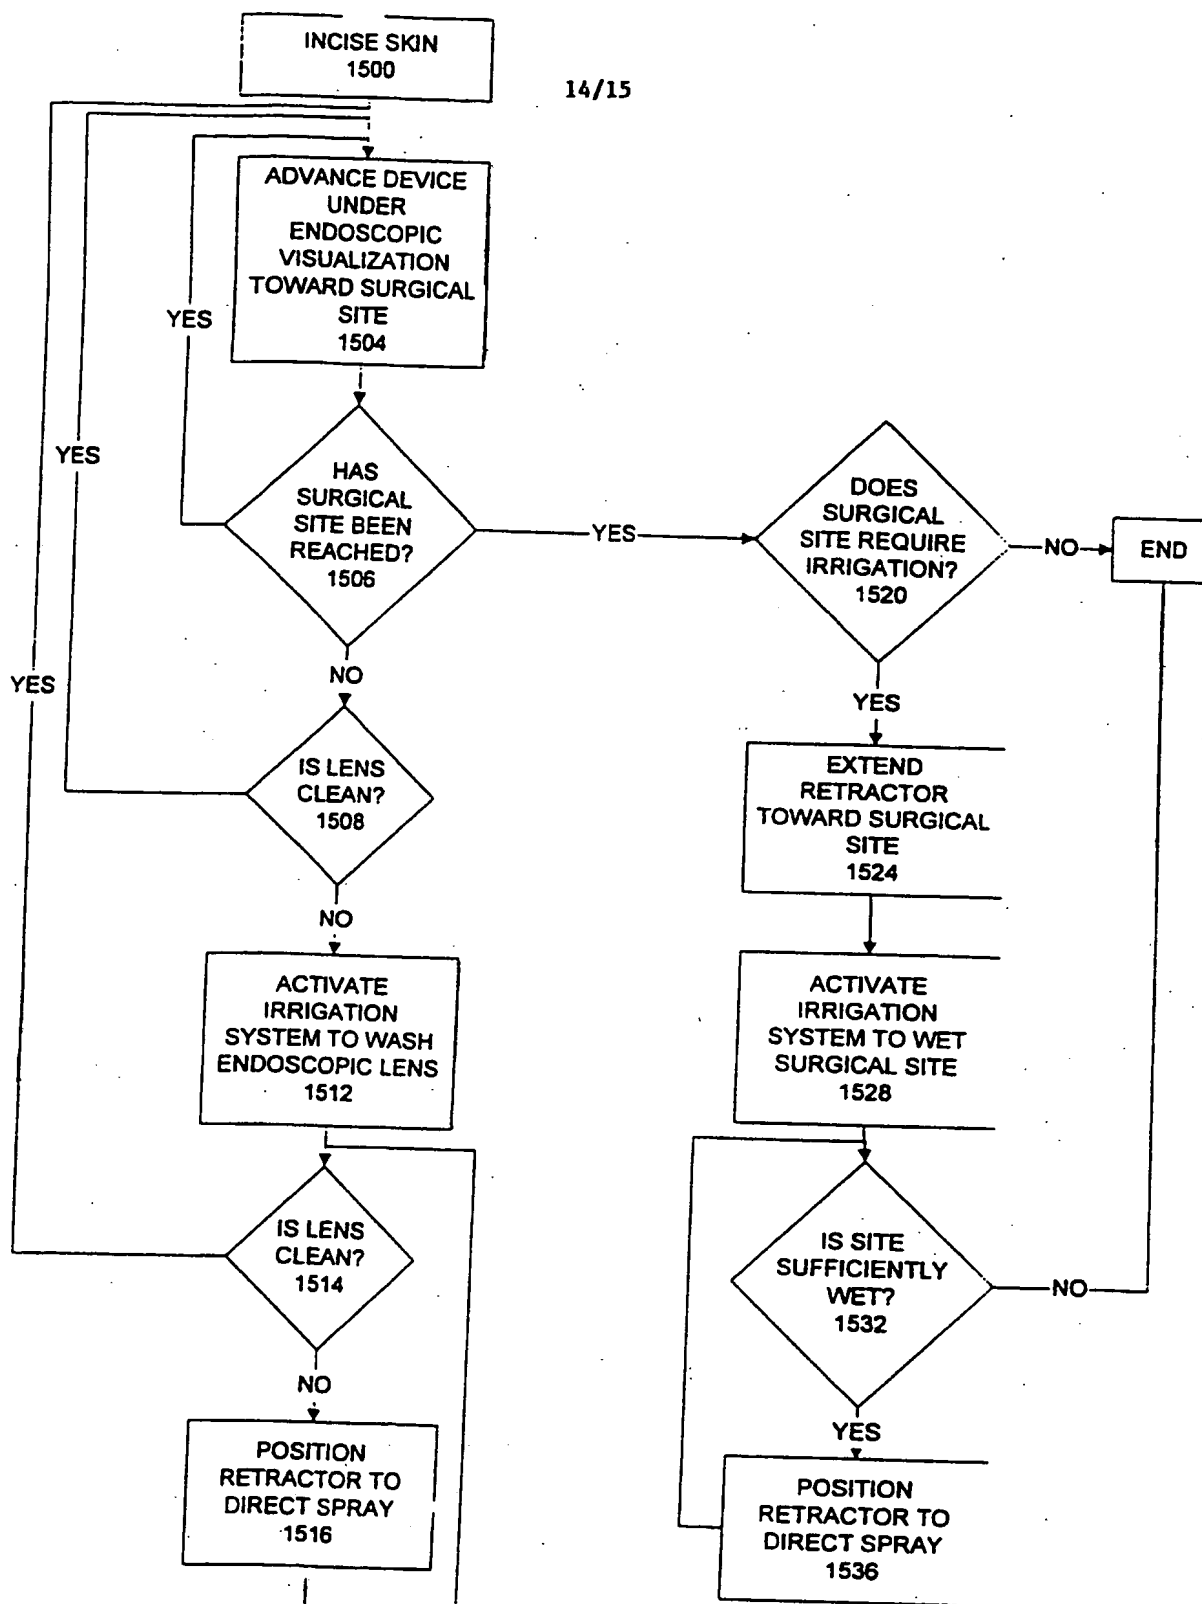


FIGURE 15

15/15

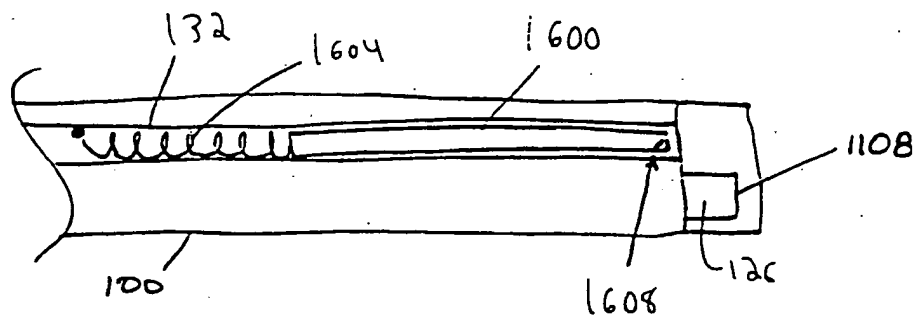


Figure 16a

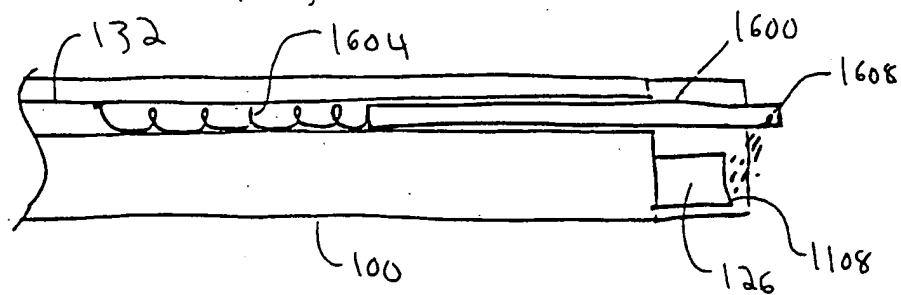


Figure 16b



## INTERNATIONAL SEARCH REPORT

Intern al Application No

PCT/US 00/00109

A. CLASSIFICATION OF SUBJECT MATTER  
 IPC 7 A61B1/12 A61B1/00

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)  
 IPC 7 A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X A	US 5 535 759 A (WILK PETER J) 16 July 1996 (1996-07-16) column 4, line 43 -column 5, line 8; figure 3	1-3,5,6 4
X	US 5 395 383 A (ADAMS RONALD D ET AL) 7 March 1995 (1995-03-07) column 5, line 50 -column 6, line 21; figure 1	1,3-6
X	US 5 630 787 A (YABE HISAO ET AL) 20 May 1997 (1997-05-20) column 7, line 64 -column 8, line 42; figure 5	9-11

☐ Further documents are listed in the continuation of box C.



Patent family members are listed in annex.

## \* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

"&" document member of the same patent family

Date of the actual completion of the international search

5 June 2000

Date of mailing of the international search report

14/06/2000

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2  
 NL - 2280 HV Rijswijk  
 Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,  
 Fax: (+31-70) 340-3016

Authorized officer

Martelli, L

# INTERNATIONAL SEARCH REPORT

International Application No. PCT/US 00 00109

FURTHER INFORMATION CONTINUED FROM PCT/ISA/ 210

This International Searching Authority found multiple (groups of) inventions in this international application, as follows:

1. Claims: 1-8

Cannula provided with irrigation lumen. An irrigation effector is slidably moveable along the axis of the cannula.

2. Claims: 9-11

Cannula provided with an endoscope lumen and an irrigation lumen.

# INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/US 00/00109

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 5535759 A	16-07-1996	US 5759187 A US 5997547 A US 5741271 A	02-06-1998 07-12-1999 21-04-1998
US 5395383 A	07-03-1995	AT 137096 T AU 662357 B AU 2706392 A BR 9204024 A CA 2080755 A,C DE 69210181 D DE 69210181 T EP 0543499 A ES 2086671 T GR 92100468 A,B IL 103442 A JP 5200047 A ZA 9208026 A	15-05-1996 31-08-1995 22-04-1993 04-05-1993 19-04-1993 30-05-1996 05-09-1996 26-05-1993 01-07-1996 30-06-1993 04-01-1998 10-08-1993 18-04-1994
US 5630787 A	20-05-1997	JP 6237883 A JP 6237884 A	30-08-1994 30-08-1994